

For 2 Tanks Oxygen and 2 Tanks Nitrous Oxide

C3000CX Manifold System, 2-O₂, N₂O
with wall model sentinel, regulators,
hoses, and tank restraints


C3000DX Manifold System, 2-O₂, N₂O
with desk model sentinel, regulators,
hoses, and tank restraints

For 2 Tanks Oxygen and 1 Tank Nitrous Oxide

C3001CX Manifold System, 2-O₂, 1-N₂O
with wall model sentinel, regulators, hoses,
and tank restraints

C3001DX Manifold System, 2-O₂, 1-N₂O
with desk model sentinel, regulators, hoses,
and tank restraints

Manifolds without Sentinel DO NOT meet the requirements of C.S.A.
Porter Instrument Company, Inc. accepts no responsibility for the installation
and/or use of manifolds without Sentinel.

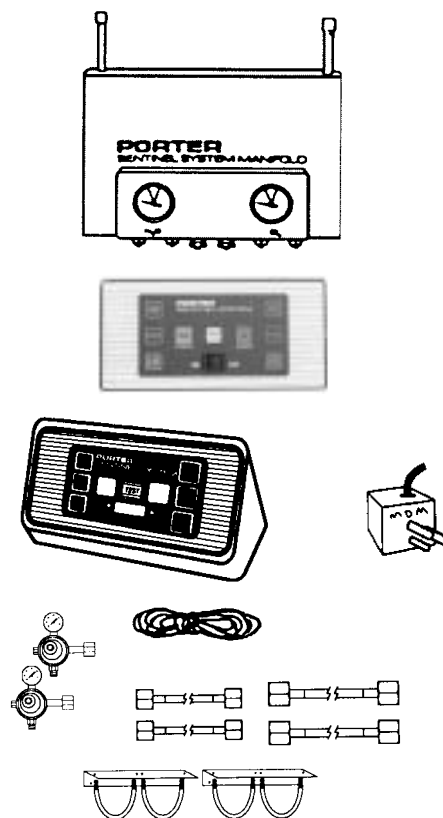


The above new manifold systems are designed to meet all requirements of
C.S.A. STANDARD Z305.1-M1992 Nonflammable Medical Gas Piping System.

Note: Order Zone Valve Separately

Zone Valves WITH CROSS + PROTECTION

C9000-1 Concealed Zone Valve for use
with concealed piping to be used
with above Sentinel Manifolds

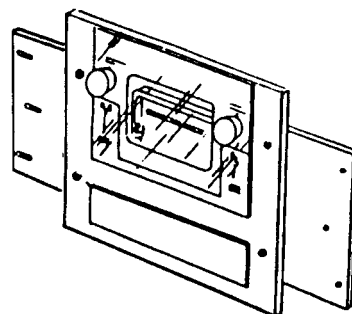

Some provinces have adopted C.S.A. STANDARD Z305.1-1992 in their Building Code.
A Zone Valve is mandatory. System installation MUST meet STANDARD requirement.